

METAL INTERFERENCES AND THEIR REMOVAL PRIOR TO THE DETERMINATION OF As(T) AND As(III) IN ACID MINE WATERS BY HYDRIDE GENERATION ATOMIC ABSORPTION SPECTROMETRY

Water-Resources Investigations Report 03-4117



U.S. Department of the Interior
U.S. Geological Survey

METAL INTERFERENCES AND THEIR REMOVAL PRIOR TO THE DETERMINATION OF As(T) AND As(III) IN ACID MINE WATERS BY HYDRIDE GENERATION ATOMIC ABSORPTION SPECTROMETRY

By R. Blaine McCleskey, D. Kirk Nordstrom, and James W. Ball

U.S. Geological Survey

Water Resources Investigations Report 03-4117

Boulder, Colorado
2003



U.S. DEPARTMENT OF THE INTERIOR
GALE A. NORTON, Secretary

U.S. GEOLOGICAL SURVEY
Charles G. Groat, Director

The use of firm, trade, and brand names in this report is for identification purposes only and does not constitute endorsement by the U.S. Geological Survey.

For additional information write to:

Chief, Branch of Regional Research
U.S. Geological Survey
Denver Federal Center
Box 25046, MS-418
Denver, Colorado 80225

Copies of this report can be purchased from:

U.S. Geological Survey
Branch of Information Services
Denver Federal Center
Box 25286
Denver, Colorado 80225-0286

CONTENTS

Abstract	2
Introduction	2
Methods of investigation	3
Sample collection and preservation	3
Reagents	3
Analytical apparatus	3
Analytical procedures	3
Determination of arsenic(T)	4
Determination of arsenic(III)	4
Removal of interfering metals prior to arsenic(III) determination	4
Results and discussion	5
Selective reduction of arsenic(III)	5
Potential metal interferences on the determination of arsenic(T)	5
Potential metal interferences on the determination of arsenic(III)	6
Cation exchange separation of iron(III) and copper	8
Accuracy and time stability of arsenic redox species in acid mine waters	8
Accuracy of arsenic(T) determinations	8
Accuracy of arsenic(III) determinations	11
Time stability of arsenic redox species	11
Summary	12
References cited	12

FIGURES

1-13. Graphs showing

1. Effect of NaBH_4 concentration on the calibration curve in solutions containing only As(III)	5
2. Effect of NaBH_4 concentration on the reduction of As(V) to As(III) in solutions containing 10 $\mu\text{g/L}$ As(III) and varying As(V) concentrations	5
3. As(T) determinations in the presence of potential interfering metals	6
4. As(T) determinations in the presence of hydride-forming metals	6
5. As(III) determinations in the presence of potential interfering metals	7
6. As(III) determinations in the presence of interfering metals	7
7. As(III) determinations in the presence of hydride-forming metals	8
8. Additive interference in the determination of As(III) in a solution containing 10 micrograms per liter As(III) and 5 milligrams per liter Cu(II)	8
9. Spike recovery determinations of As(T) using hydride generation atomic absorption spectrometry	9
10. As(T) determinations by inductively coupled plasma-optical emission spectrometry and hydride generation atomic absorption spectrometry for 20 samples collected from Summitville Mine, Colo., 6 samples collected from Richmond Mine, Calif., and 3 samples collected from the Penn Mine, Calif.	9

11. Spike recovery determinations using hydride generation atomic absorption spectrometry for As(III) in samples separated by cation exchange and not separated	11
12. As(III) determinations using hydride generation atomic absorption spectrometry for samples collected from the Summitville Mine	11
13. Time stability of As(III) for 45 surface and ground water samples from Yellowstone National Park, Wyo.; Questa Mine site, N. Mex.; Summitville Mine site, Colo.; Richmond Mine, Calif.; Penn Mine, Calif.; Ester Dome, Alaska; Fallon, Nev.; Mojave Desert, Calif.; and Kamchatka, Russia reanalyze 3 to 15 months after the initial determination. The curved line is a Gaussian Fit	12

TABLES

1. Cation exchange separation of Cu and Fe(III)	9
2. Composition of acid mine water samples collected from Summitville Mine, Colo.; Richmond Mine, Calif.; and Penn Mine, Calif.	10
3. As(T) determinations in U.S. Geological Survey standard reference water samples	10

Explanation of abbreviations

---	(not analyzed or not measured)	meq/mL	(milliequivalents per milliliter)
°C	(degrees Celsius)	mg/L	(milligrams per liter)
AAS	(atomic absorption spectrometry)	min.	(minute)
As(III)	(arsenic(III) or arsenite)	mL	(milliliters)
As(V)	(arsenic(V) or arsenate)	mv	(millivolt)
As(T)	(total arsenic (As(III) plus As(V))	MPV	(most probable value)
cm	(centimeter)	μL	(microliter)
conc.	(concentration)	μm	(micrometer)
EDL	(electrodeless discharge lamp)	μS/cm	(microsiemens per centimeter at 25 degrees Celsius)
FIAS	(flow injection analysis system)	n	(number of analyses)
g	(gas)	NaBH ₄	(sodium borohydride)
HCl	(hydrochloric acid)	nm	(nanometer)
HGAAS	(hydride generation-atomic absorption spectrometry)	RSD	(relative standard deviation)
HNO ₃	(nitric acid)	s	(standard deviation)
KI	(potassium iodide)	SRWS	(standard reference water sample)
ICP-OES	(inductively coupled plasma-optical emission spectrometry)	v/v	(volume per volume)
ISE	(ion-selective electrode)	w/v	(weight per volume)
μg/L	(micrograms per liter)	w/w	(weight per weight)
M	(moles per liter)		
meq/L	(milliequivalents per liter)		

METAL INTERFERENCES AND THEIR REMOVAL PRIOR TO THE DETERMINATION OF As(T) AND As(III) IN ACID MINE WATERS BY HYDRIDE GENERATION ATOMIC ABSORPTION SPECTROMETRY

By R. Blaine McCleskey, D. Kirk Nordstrom, and James W. Ball

ABSTRACT

Hydride generation atomic absorption spectrometry (HGAAS) is a sensitive and selective method for the determination of total arsenic (arsenic(III) plus arsenic(V)) and arsenic(III); however, it is subject to metal interferences for acid mine waters. Sodium borohydride is used to produce arsine gas, but high metal concentrations can suppress arsine production.

This report investigates interferences of sixteen metal species including aluminum, antimony(III), antimony(V), cadmium, chromium(III), chromium(IV), cobalt, copper(II), iron(III), iron(II), lead, manganese, nickel, selenium(IV), selenium(VI), and zinc ranging in concentration from 0 to 1,000 milligrams per liter and offers a method for removing interfering metal cations with cation exchange resin. The degree of interference for each metal without cation-exchange on the determination of total arsenic and arsenic(III) was evaluated by spiking synthetic samples containing arsenic(III) and arsenic(V) with the potential interfering metal. Total arsenic recoveries ranged from 92 to 102 percent for all metals tested except antimony(III) and antimony(V) which suppressed arsine formation when the antimony(III)/total arsenic molar ratio exceeded 4 or the antimony(V)/total arsenic molar ratio exceeded 2. Arsenic(III) recoveries for samples spiked with aluminum, chromium(III), cobalt, iron(II), lead, manganese, nickel, selenium(VI), and zinc

ranged from 84 to 107 percent over the entire concentration range tested. Low arsenic(III) recoveries occurred when the molar ratios of metals to arsenic(III) were copper greater than 120, iron(III) greater than 70, chromium(VI) greater than 2, cadmium greater than 800, antimony(III) greater than 3, antimony(V) greater than 12, or selenium(IV) greater than 1. Low recoveries result when interfering metals compete for available sodium borohydride, causing incomplete arsine production, or when the interfering metal oxidizes arsenic(III).

Separation of interfering metal cations using cation-exchange prior to hydride-generation permits accurate arsenic(III) determinations in acid mine waters containing high concentrations of interfering metals. Stabilization of the arsenic redox species for as many as 15 months is demonstrated for samples that have been properly filtered and acidified with HCl in the field. The detection limits for the method described in this report are 0.1 micrograms per liter for total arsenic and 0.8 micrograms per liter for arsenic(III).

INTRODUCTION

Accurate determination of the redox state of dissolved As is important for interpreting its toxicity and mobility in the environment. Dissolved As can form aqueous species in several oxidation states, but in natural waters occurs dominantly as the inorganic oxyanions As(III) and As(V).

Several analytical methods use hydride generation to selectively measure As redox species, but high metal concentrations can interfere with the determination of As(T) (As(III) plus As(V)) and As(III) (Smith, 1975; Welz and Melcher, 1984; Welsch and others, 1990; Creed and others 1996; Hageman and Welsch, 1996). Accurate determination of arsenic redox species in acid mine waters is challenging because of elevated metal concentrations frequently found in this type of water (Nordstrom and Alpers, 1999). Sixteen metal species including Al, Cd, Co, Cr(III), Cr(VI), Cu(II), Fe(II), Fe(III), Mn, Ni, Pb, Sb(III), Sb(V), Se(IV), Se(VI), and Zn were evaluated as possible interferents on the determination of As(T) and As(III). Because As(III) and As(V) exist as oxyanions in solution, interfering metal cations can be removed from solution using cation-exchange while maintaining the existing As(III) and As(T) concentrations. Pre-analysis separation of Fe(III) using cation-exchange resin for the determination of As redox species by ion chromatography in iron sulfate-sulfuric acid media has been successfully performed (Tan and Dutrizac, 1985). Cyanide also has been used as a complexing agent to eliminate interferences by metals in the determination of As using hydride-generation (Jamoussi and others, 1996). Interferences usually associated with atomic absorption analysis are negligible because arsine ($\text{AsH}_3(\text{g})$) is separated from the sample matrix.

Results of accurate and precise analytical methods can be invalidated by deteriorated samples. Proper filtration and preservation are critical for maintaining the existing As(III)/As(T) ratio prior to analyses. Wing and others (1987) observed that filtration (0.1- μm or 0.45- μm), acidification with HCl, and storage in the dark at 4°C effectively preserved the As redox species for up to 8 months in ground waters collected near Fallon, Nev. Except for Fe(III) and hydrogen sulfide (H_2S), laboratory studies demonstrate that rates of oxidation of As(III)

and reduction of As(V) in aqueous solution with redox agents common to natural waters are slow (Cherry and others, 1979). Filtering the sample removes colloidal material and bacteria that can affect the dissolved As(III)/As(T) ratio (Gihring and others, 2001; Wilkie and Hering, 1998). Acidification prevents precipitation of Fe hydroxides that can coprecipitate or adsorb As (Gao and others, 1988; Wilkie and Hering, 1996). Excluding light inhibits potential photochemical reactions (Emett and Khoe, 2001; Hug and others, 2001) and storing the samples at 4°C slows chemical reactions.

To address the need for more accurate determinations of As(T) and As(III) by hydride generation atomic absorption spectrometry (HGAAS), the U.S. Geological Survey (USGS) evaluated metal interferences and their removal in acid mine waters. This report (1) describes sample collection, preservation, and analytical procedures for the accurate determination of As(T) and As(III) using HGAAS; (2) identifies metals and the concentration at which each interferes in the determination of As(T) and As(III); (3) demonstrates that Cu(II) and Fe(III), both of which interfere in the determination of As(III) by HGAAS, can be removed from solutions using cation-exchange while maintaining existing As(III)/As(T) ratios; (4) applies the method to acid mine waters collected from the Summitville Mine, Colo.; Penn Mine, Calif.; and Richmond Mine, Calif.; and (5) presents As redox species time stability data for 45 surface- and ground-water samples collected during 1999-2002 from Yellowstone National Park, Wyo.; Questa Mine site, N. Mex.; Summitville Mine site, Colo.; Richmond Mine, Calif.; Penn Mine, Calif.; Ester Dome, Alaska; Fallon, Nev.; Mojave Desert, Calif.; and Kamchatka, Russia.

METHODS OF INVESTIGATION

Sample Collection and Preservation

Water samples collected in the field were pumped from the source through a 0.1 μm tortuous-path filter, acidified to pH less than 2 with hydrochloric acid (typically 2 mL 6-M HCl per 250 mL sample), and stored in acid-washed opaque bottles at 4°C (To and others, 1999).

Reagents

All reagents were of purity at least equal to the reagent-grade standards of the American Chemical Society. Double-distilled water and re-distilled or trace metal grade acids were used in all preparations. The following reagents were used for the As(T) and As(III) HGAAS procedure: 10 percent (w/v) KI from Aldrich; 10 percent (w/v) L-Ascorbic Acid from Aldrich; NaOH from Fisher; NaBH_4 from Fisher; trace metal grade HCl from Fisher, Assay w/w 35 to 38 percent; 1,000 mg/L As(III) from High Purity Standards; 1,000 mg/L As(V) from High Purity Standards; and cation-exchange resin, AG 50W-X8, 20-50 mesh, H^+ form from Bio-Rad.

The following single-element standards (1 to 10,000 mg/L) were prepared for interference studies: $\text{CuSO}_4 \cdot 5\text{H}_2\text{O}$ was used to prepare Cu(II); $\text{FeSO}_4 \cdot 7\text{H}_2\text{O}$ was used to prepare Fe(II); $\text{Fe}_2(\text{SO}_4)_3$ was used to prepare Fe(III); $\text{Zn}(\text{NO}_3)_2 \cdot 6\text{H}_2\text{O}$ was used to prepare Zn(II); $\text{MnSO}_4 \cdot \text{H}_2\text{O}$ was used to prepare Mn(II); $\text{Al}(\text{NO}_3)_3 \cdot 9\text{H}_2\text{O}$ was used to prepare Al(III); $\text{Ni}(\text{SO}_4) \cdot 6\text{H}_2\text{O}$ was used to prepare Ni(II); $\text{CrCl}_3 \cdot 6\text{H}_2\text{O}$ was used to prepare Cr(III); $\text{K}_2\text{Cr}_2\text{O}_7$ was used to prepare Cr(VI); $\text{CoCl}_2 \cdot 6\text{H}_2\text{O}$ was used to prepare Co(II); Cd powder was used to prepare Cd(II); NaSeO_4 was used to prepare Se(VI); Sb_2O_3 was used


to prepare Sb(III); SbCl_5 was used to prepare Sb(V); and Pb metal was used to prepare Pb. The Se(IV) standard was prepared by adding an equal volume of concentrated HCl to a portion of Se(VI) standard and heating at 90°C for 20 minutes.

Analytical Apparatus

An atomic absorption spectrophotometer (Perkin-Elmer (PE) – AAnalyst 300) with an electrically heated quartz cell having a path length of 15-cm inline with a flow injection analysis system (FIAS; PE – FIAS 100), an autosampler (PE – AS90), and an arsenic electrodeless discharge lamp (EDL) attached to an EDL power supply (PE – EDL System 2) were used. The following spectrometer parameters were used: EDL current: 380 mv; wavelength: 193.7 nm; slit: 0.7 nm. Peak height was used for data processing. The following FIAS parameters were used: carrier gas: Ar; cell temperature: 900°C; sample loop: 500 μL ; carrier solution: 10 percent (v/v) HCl; reducing agent: 0.25 percent (As(T)) or 0.03 percent (As(III)) NaBH_4 in 0.05 percent NaOH; carrier solution flow rate: 10 mL/min; reductant flow rate: 5 mL/min. Sodium borohydride was prepared daily and filtered through a 0.45 μm polyvinylidene fluoride filter membrane using a vacuum pump.

Analytical Procedures

Hydride formation occurs when As(III) in an acidic solution reacts with NaBH_4 according to the following reaction:



For the determination of As(T), As(V) is pre-reduced to As(III) using KI and L-ascorbic acid.

All water samples and standards were prepared in 25-mL volumetric flasks. The method detection limits of the HGAAS analytical procedure used at the USGS National Research Laboratory in Boulder, Colo., are 0.1 µg/L for As(T) and 0.8 µg/L for As(III).

Determination of Arsenic(T)

1. A solution containing 10 percent (w/v) KI and 10 percent (w/v) L-ascorbic acid was prepared.
2. To each 25-mL volumetric flask, 5 mL concentrated HCl and 2.5 mL of the KI-L-ascorbic acid solution prepared from step 1 were added.
3. The As(III) standard stock solution was used to prepare standards ranging in concentration from 0 to 10 µg/L As.
4. To demonstrate completeness of reduction, synthetic samples containing varying As(III)/As(V) ratios were prepared.
5. A volume of sample (up to 16.5 mL) that will yield 1 to 10 µg/L As(T) when diluted to volume was transferred to a 25-mL volumetric flask.
6. Appropriate spike-recovery samples were prepared by adding both As(III) and As(V) to selected samples to demonstrate reduction of As(V) and AsH₃(g) production.
7. The HGAAS analyses were performed a minimum of 30 minutes after sample preparation.

Determination of Arsenic(III)

1. Twenty-five mL of concentrated HCl was added to each 25-mL volumetric flask.
2. As(III) standards ranging in concentration from 0 to 20 µg/L were prepared.
3. To demonstrate that As(V) was not reduced, synthetic samples were prepared containing several As(III)/As(V) ratios.
4. A volume of sample (up to 24.75 mL) that will yield 2 to 20 µg/L As(III) when diluted to volume was transferred to a 25-mL volumetric flask.
5. Appropriate spike-recovery samples were prepared by adding both As(III) and As(V) to demonstrate that As(V) is not reduced and that adequate AsH₃(g) production occurs.
6. The HGAAS analysis was performed immediately.

Removal of Interfering Metals Prior To Arsenic(III) Determination

For samples having a Cu(II)/As(III) molar ratio greater than 120, Fe(III)/As(III) molar ratio greater than 70, Cd/As(III) molar ratio greater than 800, or for samples with low As(III) spike recoveries, the sample was mixed with cation-exchange resin (AG 50W-X8, 20-50 mesh, H⁺ form) to remove interfering metals prior to determination of As(III). The following procedure was used to remove interfering metals and regenerate the resin:

1. Approximately 100 grams dry resin was transferred to a 250-mL polyethylene bottle. The resin was washed 2 times with 100 mL 2-M HCl

- followed by 5 washes with distilled water. The excess water was decanted.
2. The resin was dried in an oven at 100°C.
 3. To a 50-mL polyethylene bottle, 12.5 grams dried resin and 25 mL sample were added. The mixture was periodically shaken for 30 minutes.
 4. The sample was separated from the resin by decanting it into an acid-washed 15-mL polyethylene bottle. This sample was used to determine the As(III) concentration.

RESULTS AND DISCUSSION

Selective Reduction of Arsenic(III)

During the As(III) determination, As(V) can be reduced to AsH₃(g) by the NaBH₄ reductant causing an overestimation of As(III) concentration. At a constant carrier concentration and FIAS flow rate, increasing the NaBH₄ concentration increases the sensitivity of the As(III) determination (fig. 1); however, when the NaBH₄ concentration exceeds 0.0625 percent, As(V) is reduced, causing an overestimation of As(III) concentration (fig. 2). To ensure selective reduction of As(III), the NaBH₄ concentration is maintained at 0.03 percent for the As(III) determination for analyses described in this report.

Potential Metal Interferences on the Determination of Arsenic(T)

Sixteen metal species including Al, Cd, Co, Cr(III), Cr(VI), Cu(II), Fe(III), Fe(II), Mn, Ni, Pb, Sb(III), Sb(V), Se(IV), Se(VI), and Zn were evaluated as possible interferents on the determination of As(T). The interference of each metal was evaluated by spiking synthetic samples containing 6 µg/L

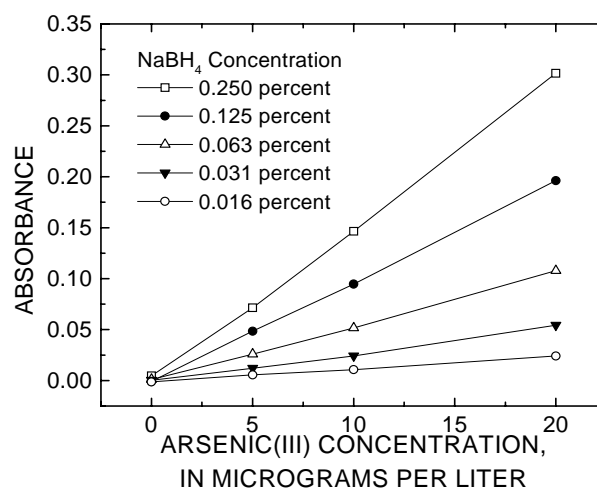


Figure 1. Effect of NaBH₄ concentration on the calibration curve in solutions containing only As(III).

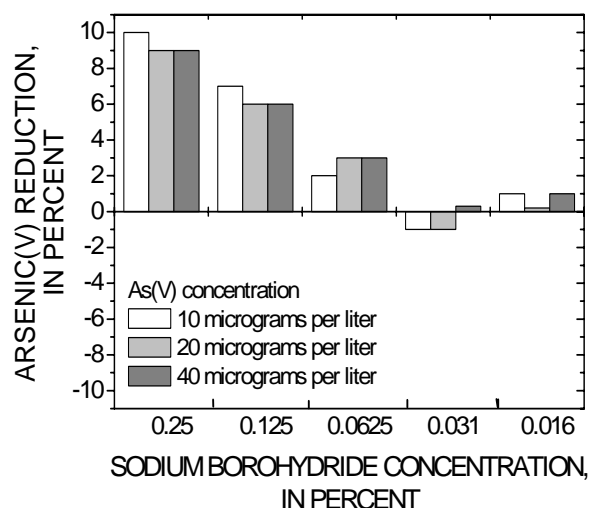


Figure 2. Effect of NaBH₄ concentration on the reduction of As(V) to As(III) in solutions containing 10 µg/L As(III) and varying As(V) concentrations.

As(III) and 6 µg/L As(V) with 0.002 to 1,000 mg/L of the potential interfering metal and then determining the As(T) concentration using the HGAAS procedure (without cation exchange treatment). Arsenic(T) recoveries ranged from 92 to 102 percent for individual solutions spiked with Al, Cd, Co, Cr(VI),

Cr(III), Cu(II), Fe(II), Fe(III), Mn, Ni, or Zn (fig. 3). For solutions spiked with a combination of metals including Al, Cd, Co, Cr(III), Cr(VI), Cu(II), Fe(II), Fe(III), Mn, Ni, and Zn, each up to a concentration of 500 mg/L, As(T) recoveries ranged from 97 to 102 percent. Dissolved Cu(II) was reduced to Cu metal during the pre-reduction step. The precipitated metal is visible at Cu concentrations greater than 100 mg/L and the liquid phase was decanted and analyzed with little change in As(T) concentration. Antimony(III) and Sb(V) were the only hydride-forming species found to interfere with the formation of $\text{AsH}_3(\text{g})$ (fig. 4). Antimony(III) and Sb(V) substantially suppressed $\text{AsH}_3(\text{g})$ formation by reacting with the NaBH_4 when the Sb(III)/As(T) molar ratio exceeded 4 or the Sb(V)/As(T) molar ratio exceeded 2. In most waters, concentrations of Sb(III) and Sb(V) are much lower than As(T) concentrations and are likely to be diluted (As(T) less than 10 $\mu\text{g/L}$) to a concentration that will not interfere with the As(T) determination. Alkali and alkaline earth elements do not interfere with the As(T) determination (Smith, 1975).

Potential Metal Interferences on the Determination of Arsenic(III)

The interference of 16 metal species on the determination of As(III) was tested by spiking synthetic samples containing 10 $\mu\text{g/L}$ As(III) and 10 $\mu\text{g/L}$ As(V) with 0.0001 to 1,000 mg/L Al, Cd, Co, Cr(III), Cr(VI), Cu(II), Fe(III), Fe(II), Mn, Ni, Pb, Sb(III), Sb(V), Se(IV), Se(VI), and Zn and determining the As(III) concentration using the HGAAS procedure (without cation-exchange treatment). Arsenic(III) recoveries for samples spiked with Al, Co, Cr(III), Fe(II), Mn, Ni, and Zn ranged from 84 to 107 percent over the entire concentration range tested (fig. 5).

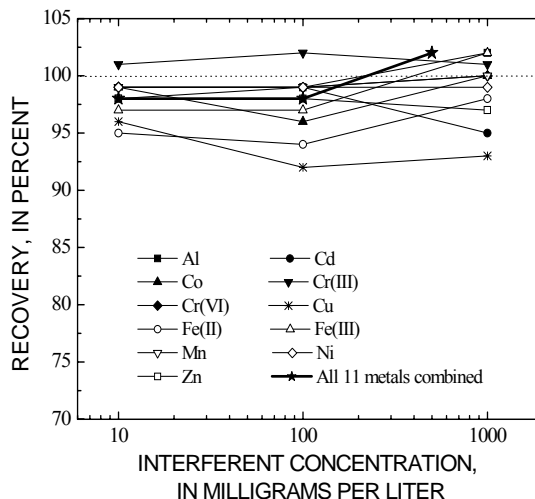


Figure 3. As(T) determinations in the presence of potential interfering metals.

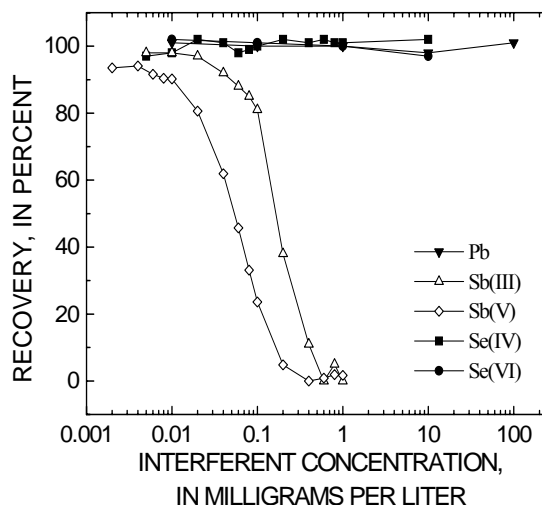


Figure 4. As(T) determinations in the presence of hydride-forming metals.

Low As(III) recoveries occurred when Cd exceeded 25 mg/L, Cr(VI) exceeded 0.03 mg/L, Cu(II) exceeded 2.0 mg/L, or Fe(III) exceeded 1.0 mg/L. Cadmium and Cu(II) are likely reduced by NaBH_4 in the FIAS reaction chamber and, consequently, arsine production is limited by the available NaBH_4 . Chromium(VI) and Fe(III) inhibit arsine production by either competing with As(III)

for the available NaBH_4 or oxidizing As(III) to As(V) . Arsenic(III) is quickly oxidized as Fe(III) undergoes photoreduction (Emett and Khoe, 2001). These synthetic samples were prepared in clear volumetric flasks and exposed to light. Therefore, the low As(III) recovery in the presence of only Fe(III) may be due to photochemical reactions with Fe(III) prior to the As(III) determination. However, when Fe(II) concentrations were twice the concentration of Fe(III) , low As(III) recoveries occurred only when Fe(III) exceeded 10 mg/L (fig. 6). Iron(II) relieves the interference from Fe(III) , within a limited Fe(III) concentration range, by reacting with free radicals generated as Fe(III) undergoes photoreduction (Emett and Khoe, 2001). Among the hydride-forming metals, Sb(III) at concentrations greater than 0.1 mg/L, Sb(V) greater than 0.4 mg/L, and Se(IV) greater than 0.02 mg/L interfered with As(III)

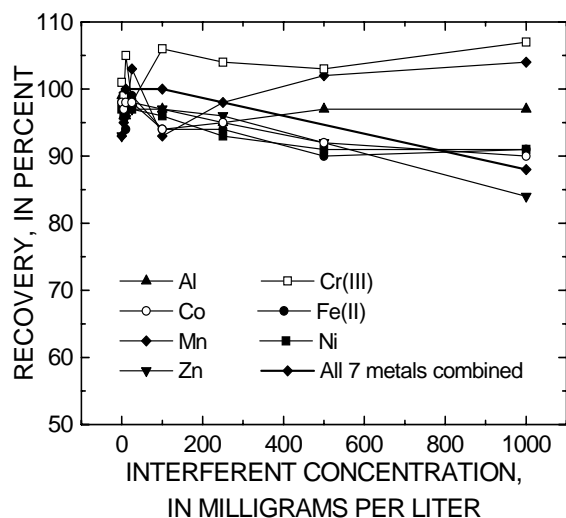


Figure 5. As(III) determinations in the presence of potential interfering metals.

determinations, whereas Pb and Se(VI) did not (fig. 7). Antimony(III), Sb(V) , and Se(IV) suppress $\text{AsH}_3(\text{g})$ production by reacting with the available NaBH_4 . An additive effect of interfering metals on the determination of As(III) was demonstrated by adding increasing amounts of Fe(III) to a solution containing 0.5 mg/L Cu and 10 $\mu\text{g/L}$ As(III) (fig. 8). Low As(III) recoveries occurred when the molar ratios of metals to As(III) were: Cu(II) greater than 120, Fe(III) greater than 70, Cr(VI) greater than 2, Cd greater than 800, Sb(III) greater than 3, Sb(V) greater than 12, or Se(IV) greater than 1. The sample could not be diluted to an As(III) concentration (As(III) less than 20 $\mu\text{g/L}$) below which these interferences were absent. Copper(II) and Fe(III) are of primary concern because water generated from acid mine drainage potentially contains high concentrations of Cu(II) and Fe(III) .

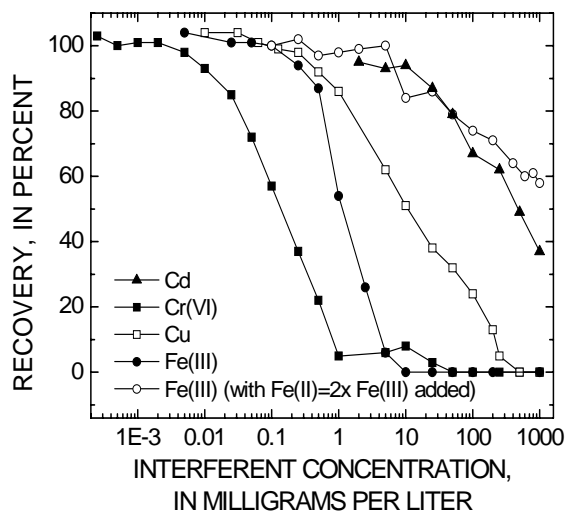


Figure 6. As(III) determinations in the presence of interfering metals.

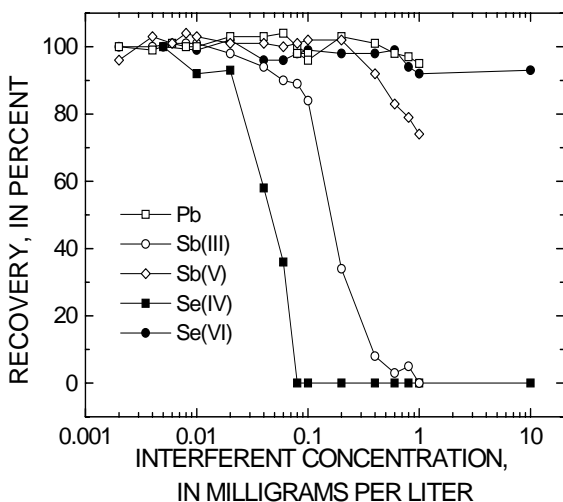


Figure 7. As(III) determinations in the presence of hydride-forming metals.

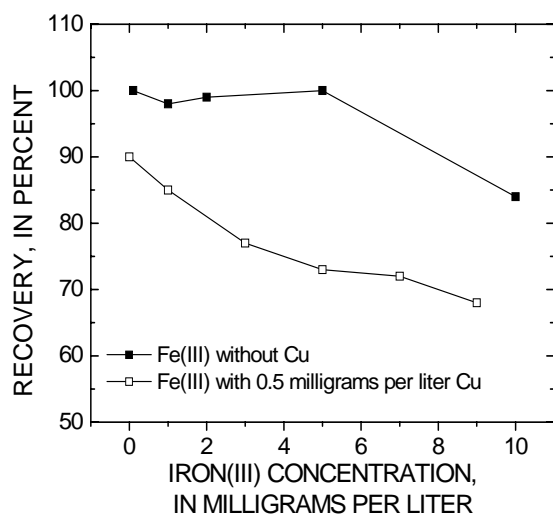


Figure 8. Additive interference in the determination of As(III) in a solution containing 10 micrograms per liter As(III) and 5 milligrams per liter Cu(II).

Cation Exchange Separation of Iron(III) and Copper

Interfering metals can be removed using cation-exchange resin prior to the determination of As(III). The relative selectivity for AG 50W-X8 cation-exchange

resin is 2.95 for Cd, 2.9 for Cu(II), and 1.0 for H^+ (Bio-Rad, 2003). Therefore, as long as the capacity of the resin (1.7 milliequivalents (meq) per mL of resin) is not exceeded, Cd and Cu(II) are expected to be removed from solution. The relative selectivity for Fe(III) is not published in the AG 50W instruction manual.

Laboratory experiments done for this report demonstrated that AG 50W-X8 cation-exchange resin in the H^+ form removed large amounts of Cu(II) and Fe(III) while maintaining the existing As(III)/As(T) ratio (table 1). When the As(III) concentration is high relative to that of the interfering metal, the sample may be diluted before analysis to a Cd, Cu(II), Cr(VI), Fe(III), Sb(III), or Se(IV) concentration that does not interfere with the As(III) determination. Chromium(VI) and the Se and Sb oxyanions will not be removed by cation exchange.

Accuracy and Time Stability of Arsenic Redox Species in Acid Mine Waters

Accuracy of Arsenic(T) Determinations

Acid mine water may contain up to 31 major metal species with concentrations that can vary over several orders of magnitude (Nordstrom and Alpers, 1999). Consequently, interferences are likely during As redox determinations by HGAAS for acid mine waters. Samples of water collected from the Reynolds Adit and a monitoring well near the Chandler Adit on the Summitville Mine site, the Richmond Mine, and the Penn Mine were analyzed for many dissolved constituents including As(T) and As(III). Concentrations of potential interfering metals for these samples are listed in Table 2. The samples contain elevated concentrations of metals, as determined using inductively coupled plasma-optical emission spectroscopy (ICP-OES) and

colorimetric determinations for Fe redox species (To and others, 1999).

Accuracy of the As(T) method was evaluated by performing a standard addition on samples collected from the Summitville Mine, Colo. (Reynolds Adit and a monitoring well near Chandler Adit); the Richmond Mine, Calif.; and the Penn Mine, Calif. Spike recoveries for the samples ranged from 96 to 101 percent (fig. 9). Twenty samples from the Summitville Mine site, 6 from the Richmond Mine, and 3 from the Penn Mine were analyzed by ICP-OES for As(T).

Concentrations compared well with As(T) concentrations determined by hydride generation (fig. 10). All As(T) determinations were performed without cation-exchange separation. As another measurement of accuracy for As(T) determinations, USGS standard reference water samples (SRWS) AMW4, T143, T155, and T159 (Farrar, 2000) were analyzed as unknowns along with the acid mine water samples. Measured concentrations compare well to the most probable values (MPV) (table 3).

Table 1. Cation exchange separation of Cu and Fe(III)

[mg/L, milligrams per liter; %, percent; ---, not measured; > greater than]

Initial Sample Concentration, mg/L					% Recovery		% Removal	
As(III)	As(V)	Cu	Fe(III)	Fe(II)	As(III)	As(T)	Cu	Fe(T)
0.010	0.010	---	---	---	96	99	---	---
0.010	0.010	25	---	---	96	97	>99	---
0.010	0.010	---	100	200	99	102	---	>99

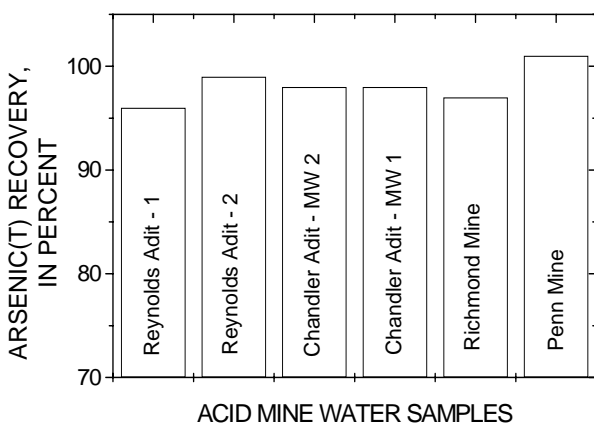


Figure 9. Spike recovery determinations of As(T) using hydride generation atomic absorption spectrometry.

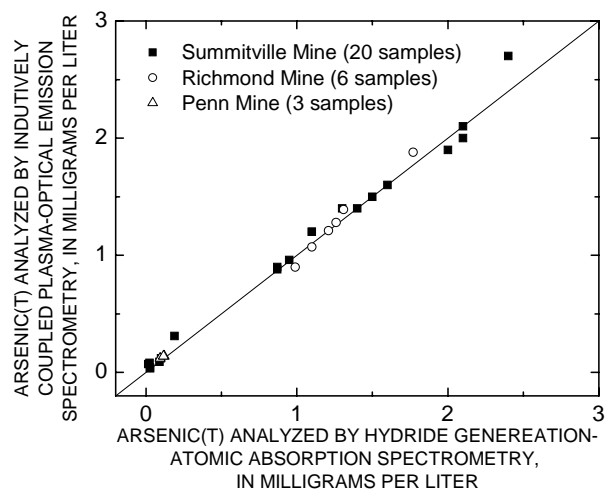


Figure 10. As(T) determinations by inductively coupled plasma-optical emission spectrometry and hydride generation atomic absorption spectrometry for 20 samples collected from Summitville Mine, Colo., 6 samples collected from Richmond Mine, Calif., and 3 samples collected from the Penn Mine, Calif.

Table 2. Composition of acid mine water samples collected from Summitville Mine, Colo.; Richmond Mine, Calif.; and Penn Mine, Calif.

[As(T), As(III) plus As(V); HGAAS, hydride generation atomic absorption spectrometry; ICP-OES, inductively coupled plasma-optical emission spectrometry; ISE, ion-selective electrode; mg/L, milligrams per liter]

Constituent mg/L	Technique	Chandler Adit Monitoring Well	Reynolds Adit	Richmond Mine	Penn Mine
pH	ISE	2.7	2.8	0.9	3.2
As(T)	ICP-OES	2.6	2.1	33	0.14
As(T)	HGAAS	2.4	2.1	35	0.12
Al	ICP-OES	170	270	1,300	5.0
Cd	ICP-OES	0.088	0.52	14	0.023
Co	ICP-OES	0.50	1.1	0.47	0.048
Cr	ICP-OES	0.13	0.088	0.27	0.070
Cu	ICP-OES	31	130	350	<0.01
Mn	ICP-OES	13	39	16	8.2
Ni	ICP-OES	0.73	1.7	1.4	0.044
Pb	ICP-OES	0.19	1.1	4.1	0.022
Zn	ICP-OES	80	35	2,100	12
Fe(II)	Colorimetric	246	707	20,700	551
Fe(III)	Colorimetric by difference	205	54	1,300	4.0

Table 3. As(T) determinations in U.S. Geological Survey standard reference water samples

[µg/L, micrograms per liter; n, number of analyses; s, standard deviation; SRWS, standard reference water samples; MPV, most probable value; %RSD, percent relative standard deviation]

SRWS	n	As(T), µg/L	s	%RSD	MPV, µg/L
AMW4	25	170	4	2	168
T143	13	15	1	6	15.2
T155	6	33	1	2	32.9
T159	23	27	1	3	28.4

Accuracy of Arsenic(III) Determinations

Accuracy of As(III) determinations, both with and without cation exchange, was estimated by spiking samples collected from the Summitville Mine (Reynolds Adit and Chandler Adit), the Richmond Mine, and the Penn Mine with As(III). Iron(III) and Cu(II) interfere with the determination of As(III) in samples collected from Summitville, but not with the Richmond or Penn Mine samples (fig 11). Spike recoveries for Summitville Mine samples not separated by cation exchange were 44 to 53 percent, whereas recoveries for the same samples separated by cation exchange were 102 to 103 percent. The Richmond and Penn Mine samples were not separated with cation exchange resin because the ratios of Fe(III) and Cu(II) to As(III) were low enough that samples could be diluted to Fe(III) and Cu(II) concentrations that did not interfere with the determination. The As(III) concentrations were underestimated in the Summitville Mine samples not separated by cation exchange (fig. 12). No USGS standard reference water sample exists for As redox species.

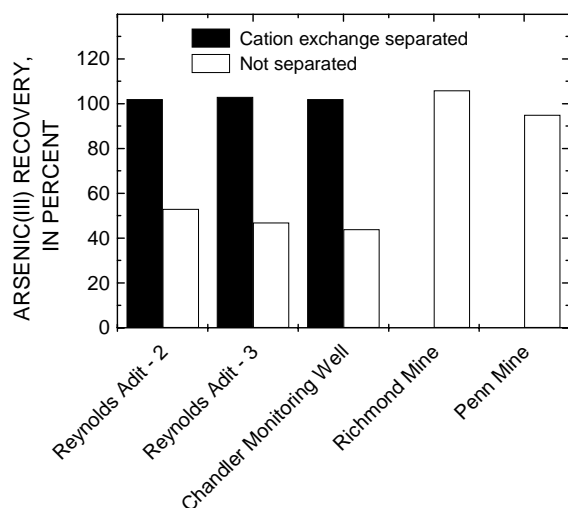


Figure 11. Spike recovery determinations using hydride generation atomic absorption spectrometry for As(III) in samples separated by cation exchange and not separated.

Time Stability of Arsenic Redox Species

The time stability of As(III) was monitored in 45 surface and ground water samples from Yellowstone National Park, Wyo.; Questa Mine site, N. Mex., Summitville Mine site, Colo., Richmond Mine, Calif., Penn Mine, Calif., Ester Dome, Alaska, Fallon, Nev., Mojave Desert, Calif., and Kamchatka, Russia. Samples were filtered through a 0.1- μ m membrane, acidified to pH <2 with HCl, and stored in opaque bottles at 4°C. Samples were reanalyzed as many as 15 months after the initial determination. The samples containing Cu(II) or Fe(III) concentrations that interfered with the As(III) determination were separated using cation exchange. The change in As(III) is represented by plotting percent difference in As(III) concentration as a function of the initial As(III)/As(T) ratio. The equation used to calculate percent difference ($\Delta\%$) is:

$$\Delta\% = \frac{(\text{Initial As(III) conc.} - \text{Final As(III) conc.}) \times 100}{\text{Initial As(III) conc.}} \quad (2)$$

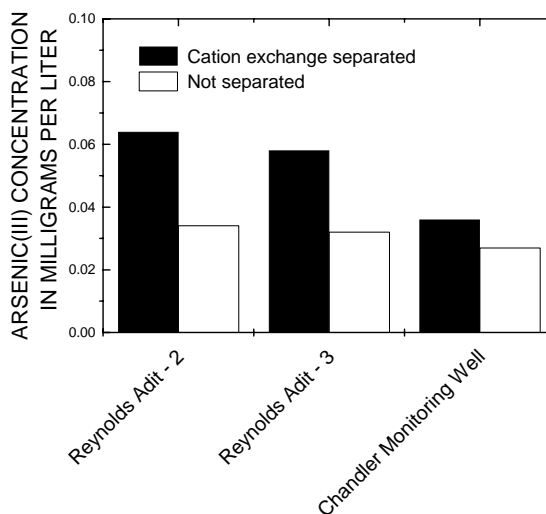


Figure 12. As(III) determinations using hydride generation atomic absorption spectrometry for samples collected from the Summitville Mine.

The As(T) concentration ranged from 0.006 to 33 mg/L and the initial As(III)/As(T) ratio ranged from 0.01 to 1.0 (fig. 13). The curved line is a Gaussian Fit. The average percent difference ($\Delta\%$) for all samples was 0.2 with a standard deviation of 7.

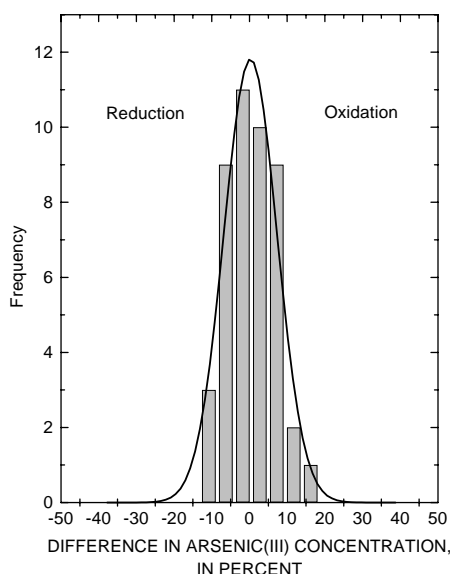


Figure 13. Time stability of As(III) for 45 surface and ground water samples from Yellowstone National Park, Wyo.; Questa Mine site, N. Mex.; Summitville Mine site, Colo.; Richmond Mine, Calif.; Penn Mine, Calif.; Ester Dome, Alaska; Fallon, Nev.; Mojave Desert, Calif.; and Kamchatka, Russia reanalyzed 3 to 15 months after the initial determination. The curved line is a Gaussian Fit.

SUMMARY

Hydride generation atomic absorption spectrometry (HGAAS) is a sensitive and selective method for the determination of As(T) and arsenic(III); however, it is subject to metal interferences for acid mine waters. Antimony(III) and Sb(V) interfere with the HGAAS As(T) determination when the molar

ratios of Sb(III) and Sb(V) exceed 4 and 2, respectively. Low As(III) recoveries occurred when the molar ratios of metals to As(III) were: Cu(II) greater than 120, Fe(III) greater than 70, Cr(VI) greater than 2, Cd greater than 800, Sb(III) greater than 3, Sb(V) greater than 12, or Se(IV) greater than 1. Samples could not be diluted to an As(III) concentration (As(III) less than 20 $\mu\text{g/L}$) below which these interferences were absent. Copper(II) and Fe(III) are of primary concern because water generated from acid mine drainage potentially contains high concentrations of Cu(II) and Fe(III). Separation of Fe(III) and Cu(II) from the sample while maintaining the existing As(III)/As(T) ratio can be achieved using cation exchange.

Some acid mine waters contain high Fe(III) and Cu(II) and accurate measurements of As(III) is problematic without removing the Fe(III) and Cu(II) prior to hydride generation. Proper sample collection and preservation are critical to maintain the existing As(III)/As(T) ratio prior to the analysis. Filtering samples through a 0.1 μm filter, acidifying with HCl to a pH less than 2, and storing in an opaque bottle at 4°C inhibits changes in the As(III)/As(T) ratios for up to 15 months after sample collection.

REFERENCES CITED

- Bio-Rad, 2003, AG 50W and AG MP-50 cation exchange resins, instruction manual: accessed April 28, 2003 at http://www.bio-rad.com/webmaster/pdfs/9118_AG_50.pdf
- Cherry, J.A., Shaikh, A.U., Tallman, D.E., and Nicholson, R.V., 1979, Arsenic species as an indicator of redox conditions in groundwater: *Journal of Hydrology*, v. 43, p. 373-392.
- Creed, J.T., Magnuson, M.L., and Brockhoff, C.A., 1996, Arsenic determination in saline waters utilizing a tubular

- membrane as a gas-liquid separator for hydride generation inductively coupled plasma mass spectrometry: *Journal of Analytical Atomic Spectrometry*, v. 11, p. 505-509.
- Emett, M.T. and Khoe, G.H., 2001, Photochemical oxidation of arsenic by oxygen and iron in acidic solutions: *Water Resources*, v. 35, p. 649-656.
- Farrar, J.W., 2000, Results of the U.S. Geological Survey's analytical evaluation program for standard reference samples distributed in October 1999: U.S. Geological Survey Open-File Report 00-227, 143 p.
- Gao, S., Tanji, K.K., and Goldberg, S., 1988, Reactivity and transformations of arsenic: Agroecosystem. *Environ.*, [Symp. 75th Annual Meeting Pac. Div., Am. Assoc. Adv. Sci.] p. 17-38.
- Gihring, T.M., Druschel, G.K., McCleskey, R.B., Hamers, R.J., and Banfield, J.F., 2001, Rapid arsenite oxidation by *Thermus aquaticus* and *Thermus thermophilus*: field and laboratory investigations: *Environmental Science and Technology*, v.35, p. 3857-3862.
- Hageman, P.L. and Welsch, E., 1996, Arsenic, antimony and selenium by flow injection or continuous flow-hydride generation-atomic absorption spectrophotometry: U.S. Geological Survey Open-File Report 96-525, p. 24-30.
- Hug, S.J., Canonica, L., Wegelin, M., Gechter, D. and Von Gunten, U., 2001, Solar oxidation and removal of arsenic at circumneutral pH in iron containing waters: *Environmental Science and Technology*, v. 35, p. 2114-2121.
- Jamoussi, B., Zafzouf, M., and Hassine, B.B., 1996, Interferences by transition metals and their elimination by cyanide as a complexing agent in the determination of arsenic using continuous flow HG-ICP-AES: *Fresenius Journal of Analytical Chemistry*, v. 356, p. 331-334.
- Nordstrom, D.K. and Alpers C.N., 1999, Negative pH, efflorescent mineralogy, and consequences for environmental restoration at the Iron Mountain Superfund site, California: *Proceedings National Academy of Science, USA*, v. 96, p. 3455-3462.
- Smith, A.E., 1975, Interferences in the determination of elements that form volatile hydrides with sodium borohydride using atomic-absorption spectrophotometry and the argon – hydrogen flame: *Analyst*, v. 100, p. 300-306.
- Tan, L.K. and Dutrizac, J.E., 1985, Determination of arsenic(V) and arsenic(III) in ferric sulfate-sulfuric acid leaching media by ion chromatography: *Analytical Chemistry*, v. 57, p. 2615-2620.
- To, T.B., Nordstrom, D.K., Cunningham, K.M., Ball, J.W., and McCleskey, R.B. 1999, New method for the direct determination of dissolved Fe(III) concentration in acid mine waters: *Environmental Science and Technology*, v. 33, p. 807-813.
- Welsch, E.P., Crock, J.G., and Sanzolone, R., 1990, Trace-level determination of arsenic and selenium using continuous-flow hydride generation atomic absorption spectrophotometry (HGAAS): U.S. Geological Survey Open-File Report 90-668, p. 38-45.
- Welz, B. and Melcher, M., 1984, Mechanisms of transition metal interferences in hydride generation atomic-absorption spectrometry. Part 2. Influence of the valence state of arsenic on the degree of signal depression caused by copper, iron and nickel: *Analyst*, v. 109, p. 573-575.
- Wilkie, J.A. and Hering, J.G., 1998, Rapid oxidation of geothermal arsenic(III) in stream waters of the Easters Sierra

- Nevada: Environmental Science and Technology, v. 32, p. 657-662.
- Wilkie, J.A. and Hering, J.G., 1996, Adsorption of arsenic onto hydrous ferric oxide; Effect of adsorbate/adsorbent ratios and co-occurring solutes: Colloids and Surfaces, v. 107, p. 97-110.
- Wing, R., Nordstrom, D.K., and Parks, G.A. 1987, Treatment of groundwater samples to prevent loss or oxidation of inorganic arsenic species: Wing, R., 1987, Analytical Characterization of Arsenic in Natural Waters, M.S. Thesis, Stanford University, p. I-1 – I-25.